

## Mouse C3b

# HK216

Edition 08-18

**ELISA KIT  
PRODUCT INFORMATION & MANUAL**

Read carefully prior to starting procedures!  
For use in laboratory research only  
Not for clinical or diagnostic use



Note that this user protocol is not lot-specific and is representative for the current specifications of this product. Please consult the vial label and the Certificate of Analysis for information on specific lots. Also note that shipping conditions may differ from storage conditions.

For research use only. Not for use in or on humans or animals or for diagnostics. It is the responsibility of the user to comply with all local/state and federal rules in the use of this product. Hycult Biotech is not responsible for any patent infringements that might result from the use or derivation of this product.

## TABLE OF CONTENTS

|  | Page |
|--|------|
| 1. Intended use .....                            | 2    |
| 2. Introduction .....                            | 2    |
| 3. Kit features .....                            | 2    |
| 4. Protocol overview .....                       | 3    |
| 5. Kit components and storage instructions ..... | 4    |
| 6. Warnings and precautions .....                | 5    |
| 7. Sample preparation .....                      | 6    |
| 8. Reagent preparation.....                      | 7    |
| 9. ELISA protocol .....                          | 9    |
| 10. Interpretation of results .....              | 10   |
| 11. Technical hints.....                         | 10   |
| 12. Quality control.....                         | 10   |
| 13. Performance characteristics .....            | 11   |
| 14. Troubleshooting .....                        | 12   |

## 1. INTENDED USE

The Mouse C3b ELISA kit is to be used for the in vitro quantitative determination of C3b in serum and plasma samples. This kit is intended for laboratory research use only and is not for use in diagnostic or therapeutic procedures.

The analysis should be performed by trained laboratory professionals.

## 2. INTRODUCTION

The complement system is an important component of innate immunity. Complement-derived products mediate functions contributing to pathogen killing and elimination. However, inappropriate activation of the system contributes to the pathogenesis of immunological and inflammatory diseases. Complement component 3 (C3) occupies a central position because of the manifold biological activities of its activation fragments, including the major fragment, C3b, which anchors the assembly of convertases effecting C3 and C5 activation. C3 is converted to C3b by proteolysis of its anaphylatoxin domain, by either of two C3 convertases. This activates a stable thioester bond, leading to the covalent attachment of C3b to cell-surface or protein-surface hydroxyl groups through transesterification. C3b is further cleaved into iC3b, C3c, C3dg and C3f. C3b and iC3b function as opsonins, they act through different complement receptors, complement receptor 1 (CD35) and complement receptor 3 (CD11b/CD18), respectively.

The mouse C3b ELISA assay is specific for the cleaved C3 fragments C3b, iC3b, and C3c, and for activated C3. Therefore, positive reactivity in plasma or serum is associated with activation of the complement cascade and C3 cleavage. In case of an acute inflammatory reaction, lots of C3 are processed into the products recognized by the assay, making this assay a useful tool for measuring the acute inflammatory response. The assay is less useful for assessing chronic inflammatory conditions since minimal reactivity may be observed. In such cases, primarily the C3dg product resides at the place of inflammation (C3c being cleared) which is not recognized by the assay. The chronic processing/activation of C3 is taking place at a lower level, which would reduce detection of the C3 fragments C3b, iC3b, and C3c. Beware that complement activity levels are mouse strain dependent and might be affected by the way the samples are collected and processed. C3 levels can differ between healthy and diseased animals, the optimal dilution can be different between these statuses.

## 3. KIT FEATURES

- Working time of 3½ hours.
- Minimum concentration which can be measured is 3.2 AU/ml.
- Measurable concentration range of 3.2 to 200 AU/ml.
- Working volume of 100 µl/well.


### Cross-reactivity

Potential cross-reacting proteins detected in the mouse C3b ELISA:

| Cross reactant | Reactivity |
|----------------|------------|
| Human          | No         |
| Rat            | No         |
| Pig            | No         |

Cross-reactivity for other species or proteins/peptides has not been tested.

#### 4. PROTOCOL OVERVIEW

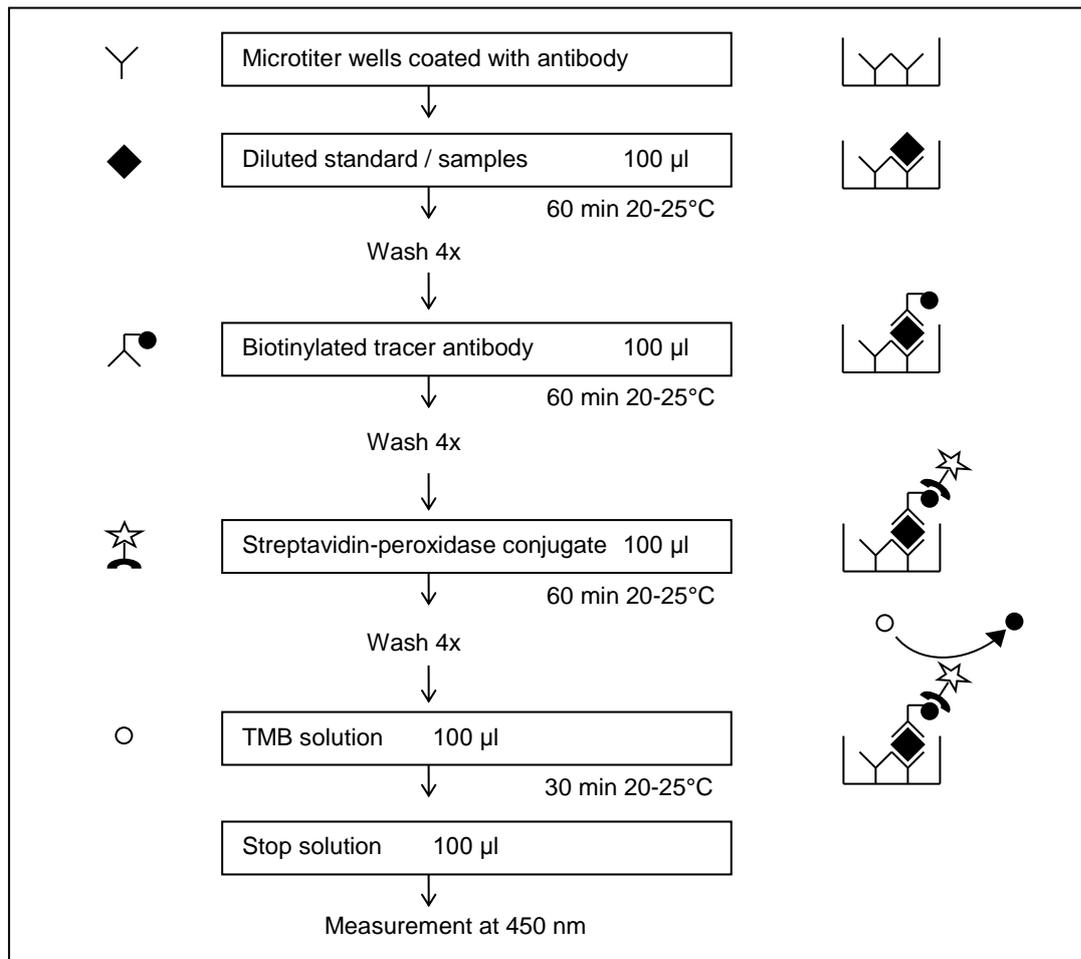

- The Mouse C3b ELISA is a ready-to-use solid-phase enzyme-linked immunosorbent assay based on the sandwich principle with a working time of 3½ hours.
- The efficient format of a plate with twelve disposable 8-well strips allows free choice of batch size for the assay.
- Samples and standards are incubated in microtiter wells coated with antibodies recognizing Mouse C3b.
- Biotinylated tracer antibody will bind to the captured Mouse C3b.
- Streptavidin-peroxidase conjugate will bind to the biotinylated tracer antibody.
- Streptavidin-peroxidase conjugate will react with the substrate, tetramethylbenzidine (TMB).
- The enzyme reaction is stopped by the addition of oxalic acid.
- The absorbance at 450 nm is measured with a spectrophotometer. A standard curve is obtained by plotting the absorbance (linear) versus the corresponding concentrations of the Mouse C3b standards (log).
- The Mouse C3b concentration of samples, which are run concurrently with the standards, can be determined from the standard curve.

## 5. KIT COMPONENTS AND STORAGE INSTRUCTIONS

| Kit component                    | Cat.#         | Quantity<br>HK216-01        | Quantity<br>HK216-02        | Color<br>code |
|----------------------------------|---------------|-----------------------------|-----------------------------|---------------|
| Wash buffer 20x                  | WB21          | 1 vial (60 ml)              | 1 vial (60 ml)              | Colorless     |
| Dilution buffer 10x              | DB101         | 1 vial (30 ml)              | 1 vial (30 ml)              | Green         |
| Standard                         |               | 2 vials, lyophilized        | 4 vials, lyophilized        | White         |
| Tracer, biotinylated             |               | 1 vials, 1 ml lyophilized   | 2 vials, 1 ml lyophilized   | White         |
| Streptavidin-peroxidase          | CON03         | 1 tube, 0.25 ml in solution | 1 tube, 0.25 ml in solution | Brown         |
| TMB substrate                    | TMB050/TMB100 | 1 vial (22 ml)              | 1 vial (22 ml)              | Brown         |
| Stop solution                    | STOP110       | 1 vial (22 ml)              | 1 vial (22 ml)              | Red           |
| 12 Microtiter strips, pre-coated |               | 1 plate                     | 2 plates                    |               |
| Certificate of Analysis          |               | 1                           | 1                           |               |
| Manual                           |               | 1                           | 1                           |               |
| Data collection sheet            |               | 1                           | 2                           |               |

Table 2

- Upon receipt, store individual components at 2 - 8°C. Do not freeze.
- Do not use components beyond the expiration date printed on the kit label.
- The standard and tracer in lyophilized form and the streptavidin-peroxidase in concentrated solution are stable until the expiration date indicated on the kit label, if stored at 2 - 8°C.
- The exact amount of the standard is indicated on the label of the vial and the Certificate of Analysis.
- The standard is single use. After reconstitution the standard cannot be stored.
- Once reconstituted the tracer is stable for one month if stored at 2 - 8°C.
- The streptavidin-peroxidase can only be stored in concentrated solution and is not stable when stored diluted.
- Upon receipt, foil pouch around the plate should be vacuum-sealed and unpunctured. Any irregularities to aforementioned conditions may influence plate performance in the assay.
- Return unused strips immediately to the foil pouch containing the desiccant pack and reseal along the entire edge of the zip-seal. Quality guaranteed for one month if stored at 2 - 8°C.

### Materials required but not provided

- Calibrated micropipettes and disposable tips.
- Distilled or de-ionized water.
- Plate washer: automatic or manual.
- Polypropylene tubes.
- Calibrated ELISA plate reader capable of measuring absorbance at 450 nm.
- Centrifuge for 1 ml tubes.

## 6. WARNINGS AND PRECAUTIONS

- For research use only, not for diagnostic or therapeutic use.
- This kit should only be used by qualified laboratory staff.
- Do not under any circumstances add sodium azide as preservative to any of the components.
- Do not use kit components beyond the expiration date.
- Do not mix reagents from different kits and lots. The reagents have been standardized as a unit for a given lot. Use only the reagents supplied by the manufacturer.
- The assay has been optimized for the indicated standard range. Do not change the standard range.
- Open vials carefully: vials are under vacuum.
- It is advised to spin down streptavidin-peroxidase tubes before use.
- Do not ingest any of the kit components.
- Kit reagents contain 2-chloroacetamide as a preservative. 2-Chloroacetamide is harmful in contact with skin and toxic if swallowed. In case of accident or if you feel unwell, seek medical advice immediately.
- The TMB substrate is light sensitive, keep away from bright light. The solution should be colorless until use.
- The stop solution contains 2% oxalic acid and can cause irritation or burns to respiratory system, skin and eyes. Direct contact with skin and eyes should be strictly avoided. If contact occurs, rinse immediately with plenty of water and seek medical advice.
- Incubation times, incubation temperature and pipetting volumes other than those specified may give erroneous results.
- Do not reuse microwells or pour reagents back into their bottles once dispensed.
- Handle all biological samples as potentially hazardous and capable of transmitting diseases.
- Hemolyzed, hyperlipemic, heat-treated or contaminated samples may give erroneous results.
- Use polypropylene tubes for preparation of standard and samples. Do not use polystyrene tubes or sample plates.

## 7. SAMPLE PREPARATION

### Collection and handling

#### Serum or plasma

Collect blood using normal aseptic techniques. Blood samples should be kept on ice. If serum is used, separate serum from blood after clotting at room temperature within one hour by centrifugation (1,500xg at 4°C for 15 min). Transfer the serum to a fresh polypropylene tube.

If plasma is used, separate plasma from blood within 20 minutes after blood sampling by centrifugation (1,500xg at 4°C for 15 min). Transfer the plasma to a fresh polypropylene tube.

#### Storage

Store samples below -20°C, preferably at -70°C in polypropylene tubes. Storage at -20°C can affect recovery of Mouse C3b. Use samples within 24 hours after thawing. Avoid multiple freeze-thaw cycles which may cause loss of Mouse C3b activity and give erroneous results. Do not use hemolyzed, hyperlipemic, heat-treated or contaminated samples. Before performing the assay, samples should be brought to room temperature (18 – 25°C) and mixed gently. Prepare all samples (controls and test samples) prior to starting the assay procedure. Avoid foaming.

### Dilution procedures

#### Serum or plasma samples

Mouse C3b can be measured if samples are diluted at least 2000x with supplied dilution buffer in polypropylene tubes. To determine the optimal dilution for your samples, an advised starting dilution for new samples is 2000x, with a further dilution step of 2x (final dilutions are 2000x, 4000x, 8000x, 16000x, etc.).

#### Comment regarding recommended sample dilution

The mentioned minimum dilution for samples should be used as a guideline. The recovery of Mouse C3b from an undiluted sample is not 100% and may vary from sample to sample. Differences in C3b levels between mouse strain and gender may be observed. For more information on this matter, please refer to the following article: *Kotimaa, J et al; "Sex matters: Systemic complement activity of female C57BL/6J and BALB/cJ mice is limited by serum terminal pathway components."* Mol Immunol 2016, 76:13. In the unlikely event that samples should be diluted less than 2000x, it is advised to run recovery experiments to determine the influence of the matrix on the detection of Mouse C3b.

Do not use polystyrene tubes or sample plates for preparation or dilution of the samples.

#### Guideline for dilution of samples

Please see table 3 for recommended sample dilutions. Volumes are based on a total volume of at least 230 µl of diluted sample, which is sufficient for one sample in duplicate in the ELISA. For dilution of samples we recommend to use at least 10 µl of sample.

|    | Dilution | Pre-dilution                | Amount of sample or pre-dilution required | Amount of dilution buffer required |
|----|----------|-----------------------------|---|------------------------------------|
| 1. | 10x      | Not necessary               | 25 µl (sample)                            | 225 µl                             |
| 2. | 20x      | Not necessary               | 15 µl (sample)                            | 285 µl                             |
| 3. | 50x      | Not necessary               | 10 µl (sample)                            | 490 µl                             |
| 4. | 100x     | Not necessary               | 10 µl (sample)                            | 990 µl                             |
| 5. | 500x     | Recommended: 10x (see nr.1) | 10 µl (pre-dilution)                      | 490 µl                             |
| 6. | 1000x    | Recommended: 10x (see nr.1) | 10 µl (pre-dilution)                      | 990 µl                             |
| 7. | 2000x    | Recommended: 20x (see nr.2) | 10 µl (pre-dilution)                      | 990 µl                             |
| 8. | 5000x    | Recommended: 50x (see nr.3) | 10 µl (pre-dilution)                      | 990 µl                             |

Table 3

## 8. REAGENT PREPARATION

Allow all the reagents to equilibrate to room temperature (20 – 25°C) prior to use. Return to proper storage conditions immediately after use.

### Wash buffer

Prepare wash buffer by mixing 60 ml of 20x wash buffer with 1,140 ml of distilled or de-ionized water, which is sufficient for 2 x 96 tests. In case less volume is required, prepare the desired volume of wash buffer by diluting 1 part of the 20x wash buffer with 19 parts of distilled or de-ionized water.

### Dilution buffer

Prepare dilution buffer by mixing 30 ml of the 10x dilution buffer with 270 ml of distilled or de-ionized water, which is sufficient for 2 x 96 tests. In case less volume is required, prepare the desired volume of dilution buffer by diluting 1 part of the 10x dilution buffer with 9 parts of distilled or de-ionized water. Concentrated dilution buffer may contain crystals. In case the crystals do not disappear at room temperature within one hour, concentrated dilution buffer can be warmed up to 37°C. Do not shake the solution.

### Standard solution

The standard is reconstituted by pipetting the amount of dilution buffer mentioned on the CoA in the standard vial. Use the standard vial as Tube 1 in Figure 1. Prepare each Mouse C3b standard in polypropylene tubes by serial dilution of the reconstituted standard with dilution buffer as shown in Figure 1\*. After reconstitution the standard cannot be stored for repeated use.

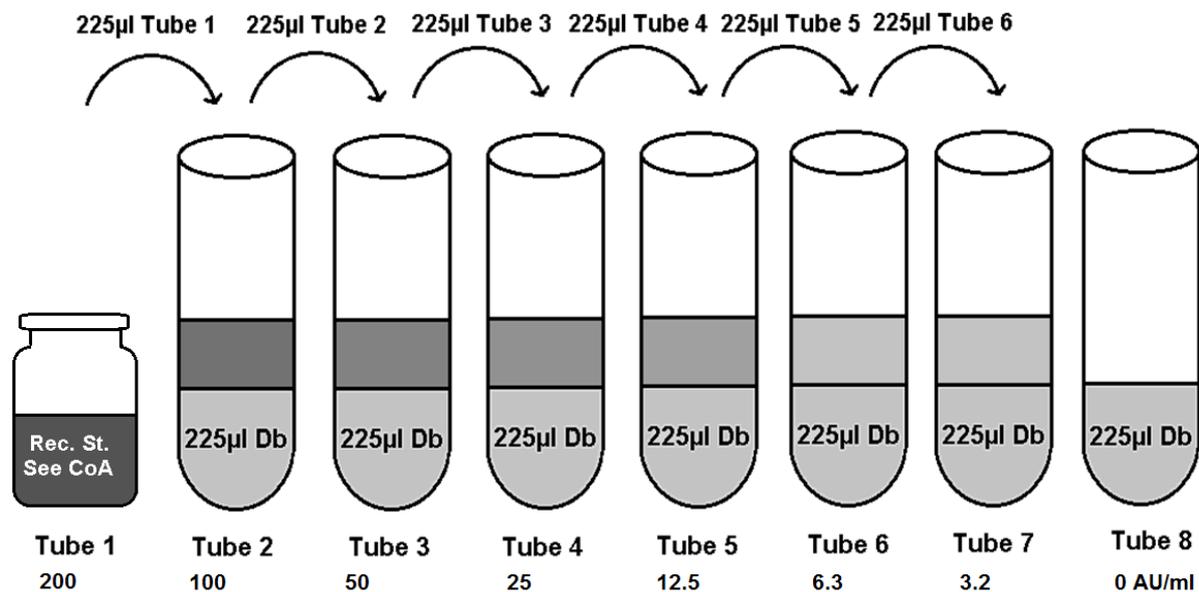


Figure 1

\*) CoA: Certificate of Analysis, St: Standard, Db: Dilution buffer

**Tracer solution**

The tracer is reconstituted by pipetting 1 ml distilled or de-ionized water. Dilute the reconstituted 1 ml tracer with 11 ml dilution buffer, which is sufficient for 1 x 96 tests. In case less volume is required, prepare the desired volume of tracer by diluting 1 part of the reconstituted tracer with 11 parts of dilution buffer.

**Streptavidin-peroxidase solution**

It is advised to spin down streptavidin-peroxidase tubes before use. Prepare the streptavidin-peroxidase solution by mixing 0.25 ml of the 100x streptavidin-peroxidase solution with 24.75 ml dilution buffer, which is sufficient for 2 x 96 tests. Where less volume is required, prepare the desired volume of streptavidin-peroxidase solution by diluting 1 part of the 100x streptavidin-peroxidase solution with 99 parts of dilution buffer.

## 9. ELISA PROTOCOL

Bring all reagents to room temperature (20 - 25°C) before use.

1. Determine the number of test wells required, put the necessary microwell strips into the supplied frame, and fill out the data collection sheet. Return the unused strips to the storage bag with desiccant, seal and store at 2 - 8°C.
2. Transfer 100 µl in duplicate of standard, samples, or controls into appropriate wells. Do not touch the side or bottom of the wells.
3. Cover the tray and tap the tray to eliminate any air bubbles. Be careful not to splash liquid onto the cover.
4. Incubate the strips or plate for 1 hour at room temperature.
5. Wash the plates 4 times with wash/dilution buffer using a plate washer or as follows\*:
  - a. Carefully remove the cover, avoid splashing.
  - b. Empty the plate by inverting plate and shaking contents out over the sink, keep inverted and tap dry on a thick layer of tissues.
  - c. Add 200 µl of wash buffer to each well, wait 20 seconds, empty the plate as described in 5b.
  - d. Repeat the washing procedure 5b/5c three times.
  - e. Empty the plate and gently tap on thick layer of tissues.
6. Add 100 µl of diluted tracer to each well using the same pipetting order as applied in step 2. Do not touch the side or bottom of the wells.
7. Cover the tray and incubate the tray for 1 hour at room temperature.
8. Repeat the wash procedure described in step 5a-e.
9. Add 100 µl of diluted streptavidin-peroxidase to each well, using the same pipetting order as applied in step 2. Do not touch the side or bottom of the wells.
10. Cover the tray and incubate the tray for 1 hour at room temperature.
11. Repeat the wash procedure described in step 5a-e.
12. Add 100 µl of TMB substrate to each well, using the same pipetting order as applied in step 2. Do not touch the side or bottom of the wells.
13. Cover the tray and incubate the tray for 30 minutes at room temperature. It is advised to control the reaction on the plate regularly. In case of strong development the TMB reaction can be stopped sooner. Avoid exposing the microwell strips to direct sunlight. Covering the plate with aluminum foil is recommended.
14. Stop the reaction by adding 100 µl of stop solution with the same sequence and timing as used in step 12. Mix solutions in the wells thoroughly by gently swirling the plate. Gently tap the tray to eliminate any air bubbles trapped in the wells.
15. Read the plate within 30 minutes after addition of stop solution at 450 nm using a plate reader, following the instructions provided by the instrument's manufacturer.

\*) In case plate washer is used, please note: use of a plate washer can result in higher background and decrease in sensitivity. We advise validation of the plate washer with the manual procedure. Make sure the plate washer is used as specified for the manual method.

## 10. INTERPRETATION OF RESULTS

- Calculate the mean absorbance for each set of duplicate standards, control and samples.
- If individual absorbance values differ by more than 15% from the corresponding mean value, the result is considered suspect and the sample should be retested.
- The mean absorbance of the zero standard should be less than 0.3.
- Create a standard curve using computer software capable of generating a good curve fit. The mean absorbance for each standard concentration is plotted on the vertical (Y) axis versus the corresponding concentration on the horizontal (X) axis (logarithmic scale).
- If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.
- Samples that give a mean absorbance above the absorbance for the highest standard concentration are out of range of the assay. These samples should be retested at a higher dilution.

## 11. TECHNICAL HINTS

- User should be trained and familiar with ELISA assays and test procedure.
- If you are not familiar with the ELISA technique it is recommended to perform a pilot assay prior to evaluation of your samples. Perform the assay with a standard curve only following the instructions.
- Improper or insufficient washing at any stage of the procedure will result in either false positive or false negative results. Completely empty wells before dispensing wash buffer, fill with wash buffer as indicated for each cycle and do not allow wells to sit uncovered or dry for extended periods.
- Since exact conditions may vary from assay to assay, a standard curve must be established for every run. Samples should be referred to the standard curve prepared on the same plate.
- Do not mix reagents from different batches, or other reagents and strips. Remainders should not be mixed with contents of freshly opened vials.
- Each time the kit is used, fresh dilutions of standard, sample, tracer, streptavidin-peroxidase and buffers should be made.
- Caps and vials are not interchangeable. Caps should be replaced on the corresponding vials.
- To avoid cross-contaminations, change pipette tips between reagent additions of each standard, between sample additions, and between reagent additions. Also, use separate reservoirs for each reagent.
- Waste disposal should be performed according to your laboratory regulations.

### Technical support

Do not hesitate to contact our technical support team at [support@hycultbiotech.com](mailto:support@hycultbiotech.com) for inquiries and technical support regarding the Mouse C3b ELISA.

Hycult Biotech, Frontstraat 2A, 5405 PB Uden, the Netherlands

T: +31 (0)413 251 335, F: +31 (0)413 248 353

## 12. QUALITY CONTROL

The Certificate of Analysis included in this kit is lot-specific and is to be used to verify results obtained by your laboratory. The absorption values provided on the certificate of analysis are to be used as a guideline only. The results obtained by your laboratory may differ.

This assay is designed to eliminate interference by soluble receptors, binding proteins, and other factors present in biological samples. Until all factors have been tested in the immunoassay, the possibility of interference cannot be excluded.

For optimal performance of this kit, it is advised to work according to good laboratory practice.

### 13. PERFORMANCE CHARACTERISTICS

#### Linearity

The linearity of the assay was determined by serially diluting samples containing mouse C3b. The diluted sample was measured in the assay. Samples were diluted at least 450 times.

| Samples                         | AU/ml  | CV(%) |
|---------------------------------|--------|-------|
| Non Swiss albino K2-EDTA plasma | 332117 | 3.1   |
| C57B6 heparin plasma            | 554266 | 3.3   |
| C57B6 citrate plasma            | 462613 | 1.1   |
| C57BL/6OlaHsd Harlan female     | 312870 | 3.3   |
| BALB/c EDTA plasma              | 19767  | 0.6   |
| BALB/c heparin plasma           | 375034 | 8.0   |
| BALB/c citrate plasma           | 758282 | 3.5   |
| CBA/caOlaHsd female serum       | 365283 | 7.6   |
| MRL Harlan male serum           | 258412 | 9.8   |

#### Recovery

Normal mouse serum samples containing baseline levels of mouse C3b, were spiked with mouse C3b, in concentrations of 31 and 250 AU/ml. Samples with and without mouse C3b were incubated for 30 minutes at room temperature and measured using the ELISA. Values for mouse C3b, ranged between 96% and 115%.

## 14. TROUBLESHOOTING

Warranty claims and complaints in respect of deficiencies must be logged before expiry date of the product. A written complaint containing lot number of the product and the generated data can be sent to support@hycultbiotech.com.

Suggestions summarized below in Table 5 can be used as guideline in case of unexpected assay results.

| Low absorbance | High absorbance | Poor duplicates | All wells positive | All wells negative | Possible cause  |
|----------------|-----------------|-----------------|--------------------|--------------------|---|
| •              | •               |                 | •                  | •                  | Kit materials or reagents are contaminated or expired                     |
| •              |                 |                 |                    |                    | Incorrect reagents used   |
| •              |                 | •               | •                  |                    | Lyophilized reagents are not properly reconstituted                       |
| •              | •               | •               | •                  | •                  | Incorrect dilutions or pipetting errors                                   |
| •              |                 | •               |                    |                    | Improper plastics used for preparation of standard and/or samples         |
| •              | •               |                 |                    |                    | Improper incubation times or temperature                                  |
|                |                 | •               |                    |                    | Especially in case of 37°C incubation: plates are not incubated uniformly |
| •              |                 |                 |                    |                    | Assay performed before reagents had reached room temperature              |
| •              | •               | •               | •                  | •                  | Procedure not followed correctly  |
|                |                 |                 |                    | •                  | Omission of a reagent or a step   |
|                |                 | •               |                    |                    | Poor mixing of samples  |
|                | •               |                 | •                  |                    | Low purity of water   |
|                | •               | •               |                    |                    | Strips were kept dry for too long during/after washing                    |
|                | •               | •               | •                  |                    | Inefficient washing   |
|                | •               | •               |                    |                    | Cross-contamination from other samples or positive control                |
|                |                 | •               | •                  |                    | TMB solution is not clear or colorless                                    |
| •              | •               |                 |                    |                    | Wrong filter in the microtiter reader                                     |
|                | •               | •               |                    |                    | Air bubbles   |
|                |                 | •               |                    |                    | Imprecise sealing of the plate after use                                  |
| •              |                 |                 |                    |                    | Wrong storage conditions  |
| •              |                 |                 |                    |                    | Lamp in microplate reader is not functioning optimally                    |

Table 5